

Scanner-Specific Variability in Neck CT Image Quality and Dose Efficiency: A Multicenter Quantitative Analysis

Hayley Cash, MS¹, Rafael Carballeira², Stephen Adjei, BE², David Pastel, MD³, Marthony Robins, PhD^{2,3}
¹Medical University of South Carolina, Charleston
²Dartmouth College, Hanover, NH
³Dartmouth Hitchcock Medical Center, Lebanon, NH

ABSTRACT

Purpose: To evaluate neck CT image quality (IQ) and dose efficiency for lesion assessment across multiple scanners, identifying scanner-level differences and protocol optimization opportunities. **Methods:** This retrospective study included 957 contrast-enhanced CT neck soft tissue exams from 12 scanners across 8 hospitals over 6 months. IQ was objectively assessed using signal-to-noise ratio (SNR) and contrast-to-noise ratio (CNR), then subjectively via a blinded reader study performed by a radiologist who rated IQ-perceptibility on a 5-point scale. The ACR's Achievable Dose (AD) (15 mGy) to Diagnostic Reference Levels (DRL) (19 mGy) coupled with the Rose Criterion was used as a standardized reference. Dose and size metrics included CTDIvol (3.94–34.61 mGy), and water-equivalent diameter (WED) (18–59 cm). Regression and ANCOVA assessed relationships between IQ, dose, and scanner type. **Results:** CTDIvol showed no significant correlation with SNR or CNR ($p>0.05$), indicating that increasing radiation dose did not yield meaningful improvements in objective noise or contrast performance. CTDIvol also demonstrated no meaningful association with radiologist perceived IQ rating ($R^2\approx0.03$, $p>0.05$), and subjective perceptibility did not significantly correlate with SNR or CNR ($p>0.05$). However, regression analysis indicates that scanner type was the primary determinant of IQ. CTDIvol varied 5-fold across scanners (4.6–22.5 mGy), but radiologist ratings varied only 1.5-fold (3.0–4.6), with high-dose scanners (>18 mGy) achieving 4.30 ± 0.14 versus 3.40 ± 0.32 for low-dose scanners.

CONTACT

Hayley Cash
Medical University of South Carolina
cashhay@musc.edu



METHODS

Study Design & Cohort Retrospective analysis of 957 contrast-enhanced neck soft tissue CT exams acquired over 6 months across 12 scanners at 8 hospitals. Scanners included Philips, Siemens (1A, 1B, 2, 3, 4, 5), and GE (1A, 1B, 2, 3, 4) platforms representing the institutional fleet. **Objective Image Quality** ROIs were placed in homogeneous soft tissue and adjacent background to compute:
$$SNR = \frac{\mu_{signal}}{\sigma_{background}}$$
$$CNR = \frac{|\mu_{signal} - \mu_{background}|}{\sigma_{background}}$$
Subjective Image Quality A blinded radiologist rated each exam on a 5-point perceptibility scale (1 = non-diagnostic, 5 = excellent). Cases were randomized and scanner identity was withheld. **Dose & Size Metrics** CTDIvol was extracted from DICOM dose reports (range: 3.94–34.61 mGy). Patient size was characterized by water-equivalent diameter (WED) computed from axial images at the level of the thyroid:

$$WED = 2 \sqrt{\frac{A_{ROI}}{\pi} \left(\frac{CT_{ROI}}{1000} + 1 \right)}$$

where A_{ROI} is the cross-sectional area and CT_{ROI} is the mean CT number in HU. WED range: 18–59 cm.

Reference Standards

ACR Achievable Dose (AD): **15 mGy**
ACR Diagnostic Reference Level (DRL): **19 mGy**
Rose Criterion for lesion detectability: **CNR $\geq$ 5**

Statistical Analysis Linear regression assessed CTDIvol vs. SNR, CNR, and radiologist rating. ANCOVA tested scanner type as a predictor of IQ while controlling for WED. Pearson correlations were computed between rating and each objective metric. Significance threshold $\alpha = 0.05$.

Results

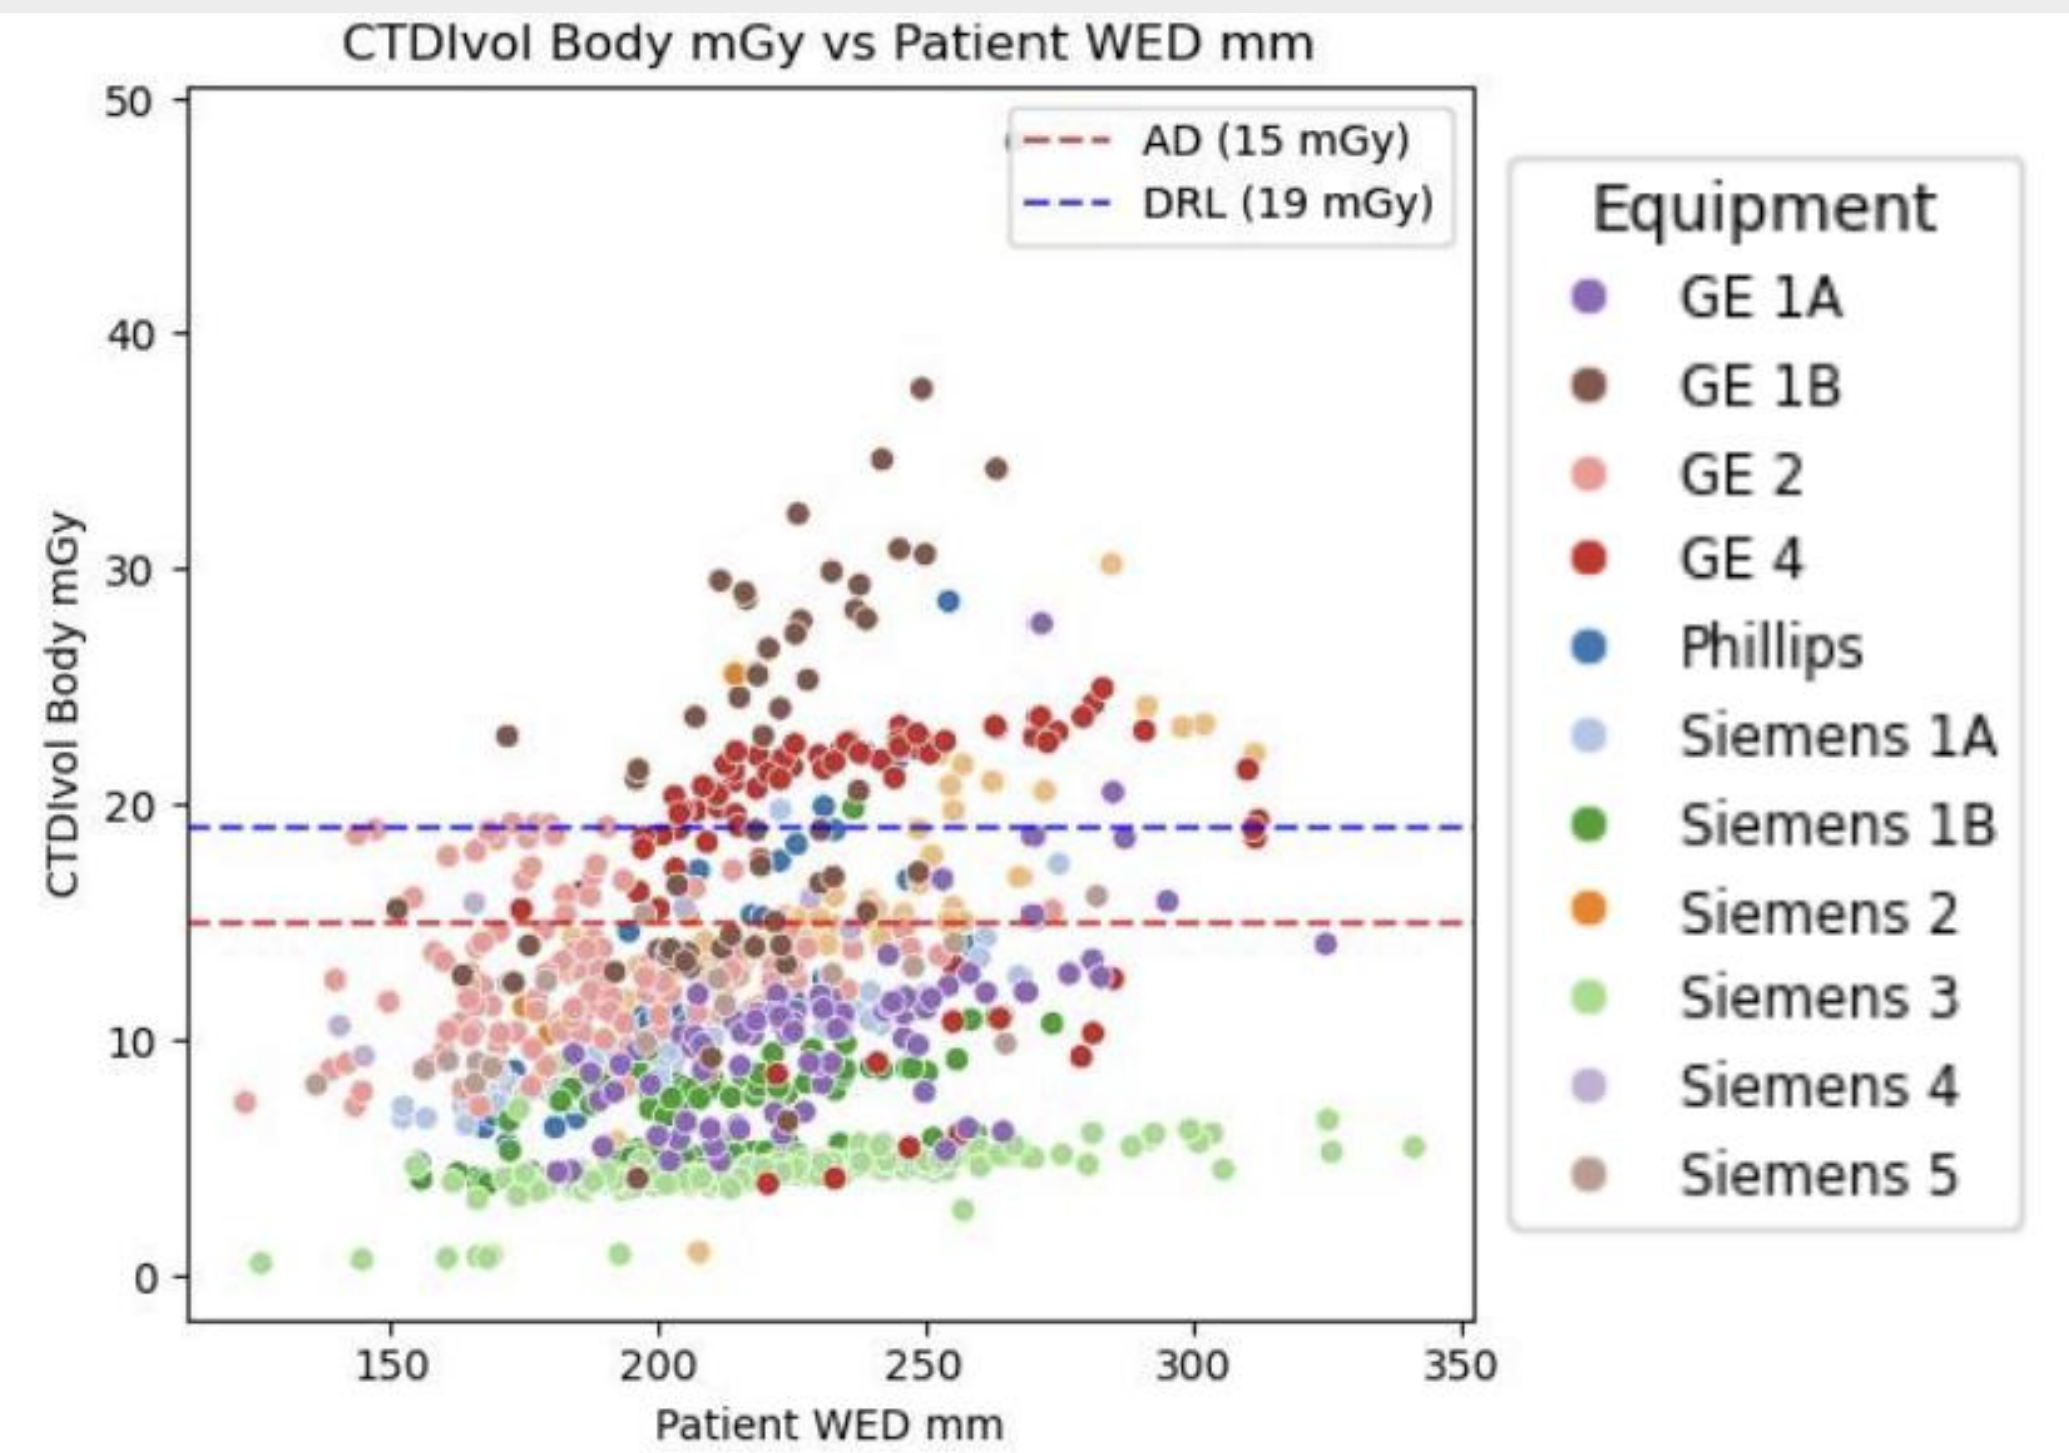


Figure 1: CTDIvol (mGy) versus patient water-equivalent diameter (WED, mm) across all scanners. CTDIvol varied up to twofold at similar WEDs, with differences driven primarily by scanner-specific protocols rather than patient size.

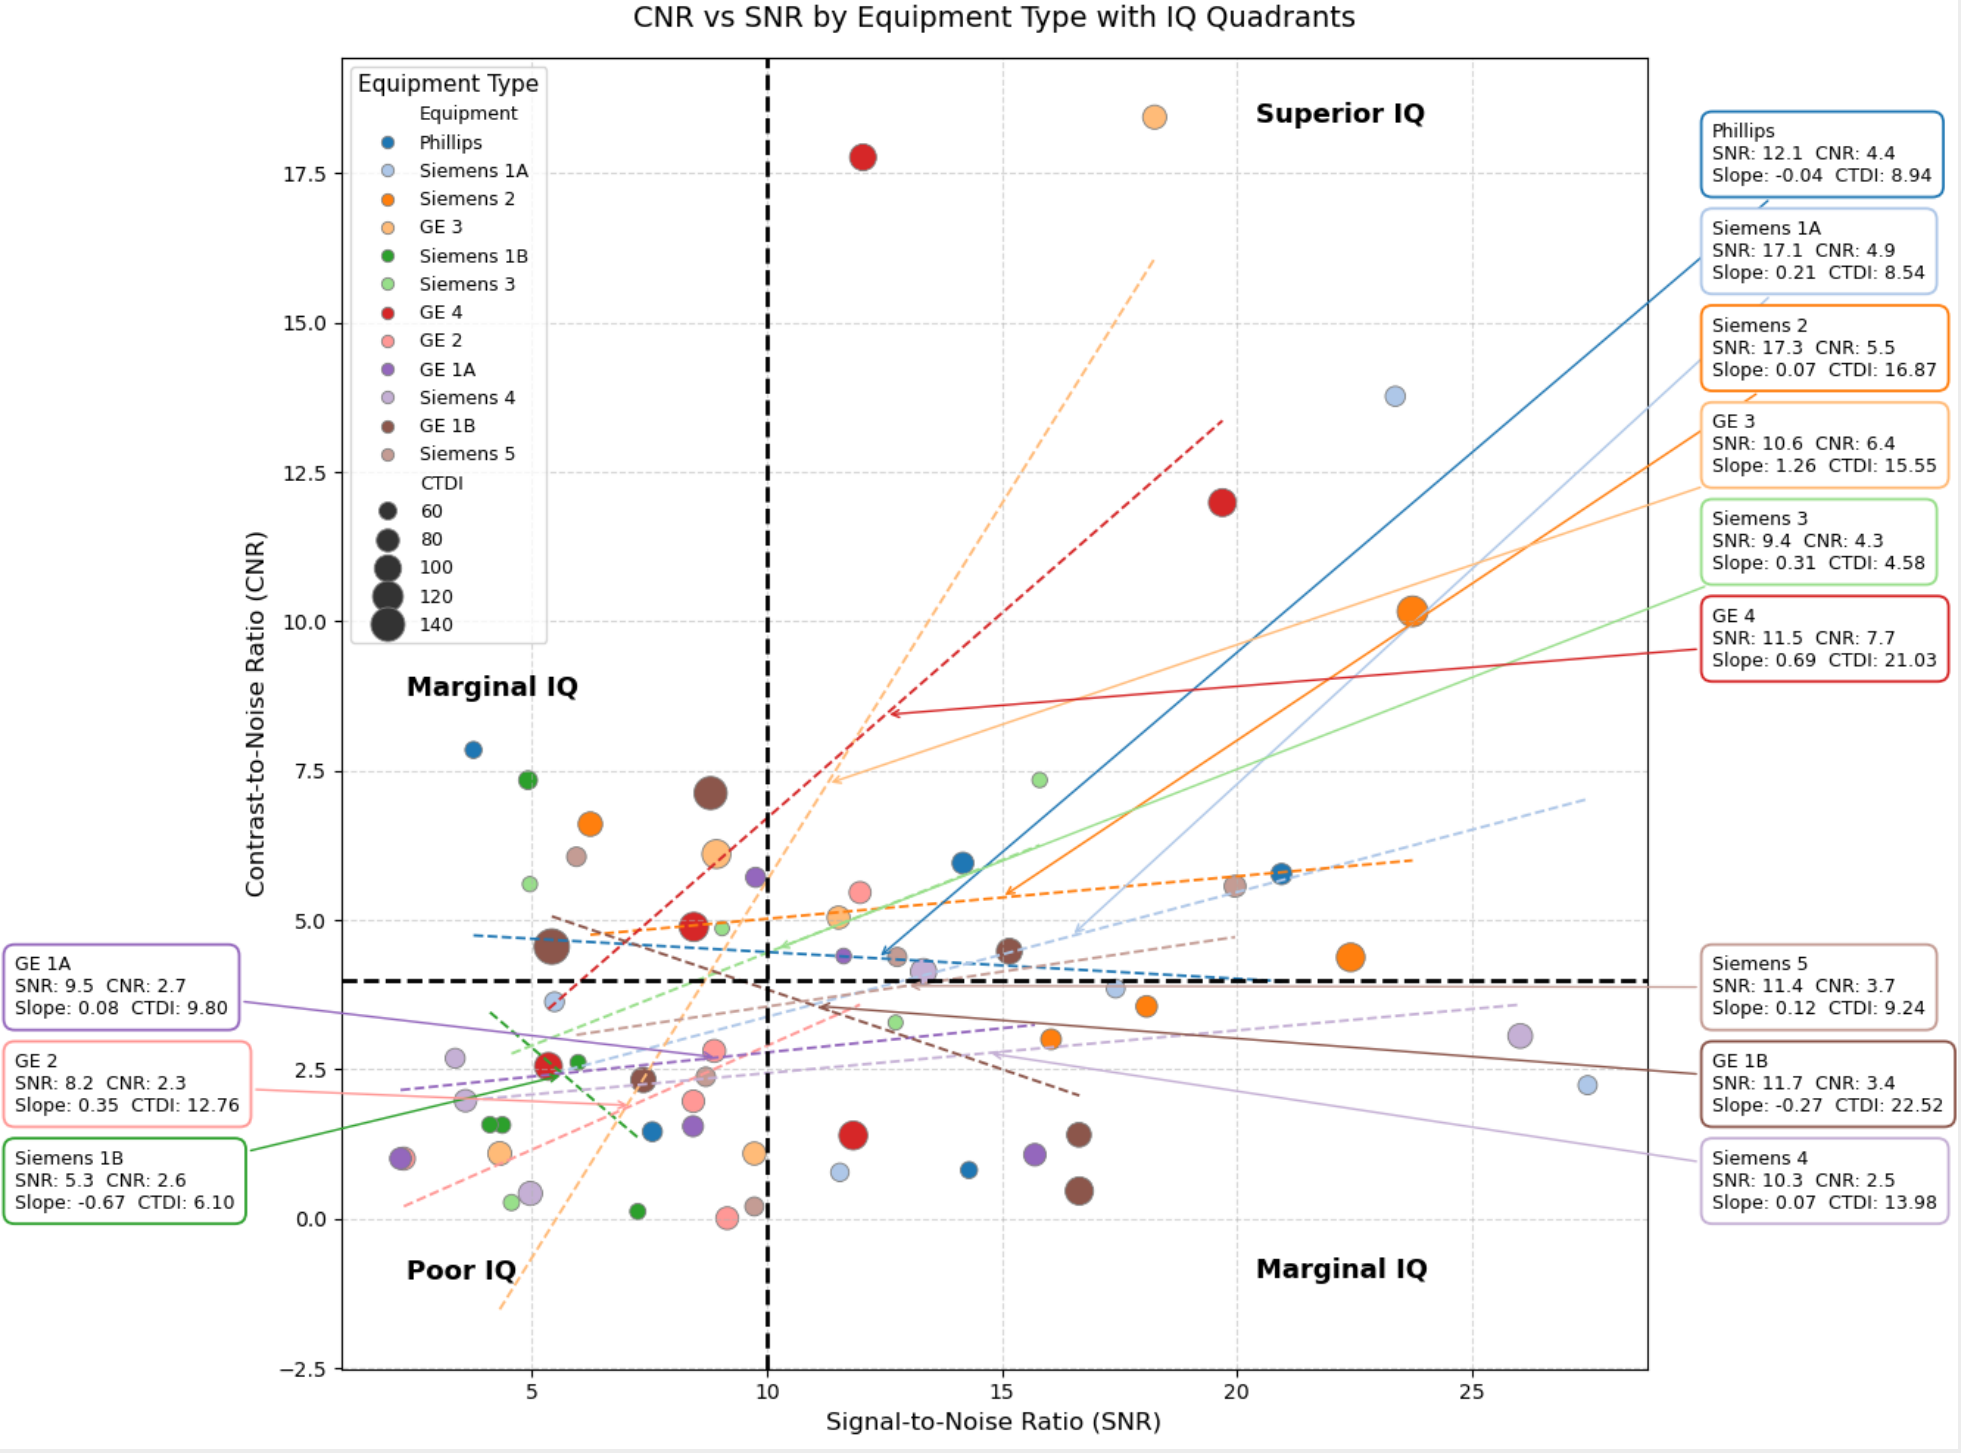


Figure 2: CNR versus SNR regression analyses by scanner type. Scannerspecific relationships varied in slope and intercept. Certain scanners achieved higher CNR at equivalent SNR independent of dose, while higher-dose scanners did not demonstrate proportional CNR gains, indicating opportunities for protocol optimization.

Equipment	CTDI (Mean $\pm$ SD)	SNR (Mean $\pm$ SD)	CNR (Mean $\pm$ SD)	Rating (Mean $\pm$ SD)
Philips	8.94 $\pm$ 2.55	12.15 $\pm$ 6.66	4.37 $\pm$ 3.07	3.2 $\pm$ 0.45
Siemens 1A	8.54 $\pm$ 0.82	17.05 $\pm$ 8.83	4.85 $\pm$ 5.13	3.8 $\pm$ 1.10
Siemens 2	16.87 $\pm$ 6.63	17.30 $\pm$ 6.92	5.54 $\pm$ 2.93	4.6 $\pm$ 0.55
Siemens 1B	6.10 $\pm$ 1.21	5.33 $\pm$ 1.29	2.65 $\pm$ 2.77	3.0 $\pm$ 0.82
Siemens 3	4.58 $\pm$ 0.57	9.43 $\pm$ 4.88	4.27 $\pm$ 2.67	3.4 $\pm$ 0.55
GE 1A	9.80 $\pm$ 2.98	9.55 $\pm$ 4.93	2.75 $\pm$ 2.17	4.2 $\pm$ 0.45
GE 2	12.76 $\pm$ 0.55	8.15 $\pm$ 3.56	2.25 $\pm$ 2.08	4.0 $\pm$ 0.00
Siemens 4	13.98 $\pm$ 3.27	10.26 $\pm$ 9.71	2.46 $\pm$ 1.38	4.4 $\pm$ 0.55
GE 1B	22.52 $\pm$ 7.89	11.68 $\pm$ 5.04	3.39 $\pm$ 2.45	4.2 $\pm$ 1.30
Siemens 5	9.24 $\pm$ 1.46	11.43 $\pm$ 5.36	3.72 $\pm$ 2.42	3.6 $\pm$ 0.89
GE 3	15.55 $\pm$ 3.72	10.55 $\pm$ 5.06	6.36 $\pm$ 7.13	3.8 $\pm$ 0.45
GE 4	21.03 $\pm$ 1.53	11.48 $\pm$ 5.35	7.72 $\pm$ 6.96	4.4 $\pm$ 0.89

Table 1. Radiation dose and image quality metrics across 12 CT scanner types. Higher CTDIvol values did not consistently correlate with improved CNR or SNR. Several lower-dose scanners demonstrated comparable or superior image quality, indicating inefficient dose utilization across platforms.

DISCUSSION

Dose and image quality are decoupled. Despite a 5-fold range in CTDIvol across scanners (4.6–22.5 mGy), radiologist ratings varied only 1.5-fold (3.0–4.6), and CTDIvol showed no significant correlation with SNR, CNR, or perceived quality. This challenges the assumption that higher dose reliably yields better diagnostic images at the neck. **Scanner type is the dominant driver.** ANCOVA identified scanner as the primary determinant of IQ after controlling for patient size. Several low-dose scanners matched or exceeded the IQ of high-dose scanners — most notably Siemens 3 (4.58 mGy, rating 3.4) achieving comparable diagnostic ratings to GE 1B (22.52 mGy, rating 4.2). Reconstruction algorithms, detector design, and protocol parameters appear to explain more IQ variance than dose itself. **Patient size does not explain the variation.** Figure 1 shows up to 2-fold CTDIvol differences at equivalent WEDs, confirming the variation is protocol-driven rather than anatomically necessary. **Clinical implications.** Many institutions deliver radiation above the ACR DRL without measurable diagnostic benefit. Conversely, scanners operating below the AD demonstrate that diagnostic-quality neck CT is achievable at substantially lower doses. A scanner-specific approach to protocol standardization — rather than a one-size-fits-all dose target — would better serve the ALARA principle. **Limitations.** Single-reader subjective scoring introduces rater variability; multi-reader validation is planned. Retrospective design precludes controlled protocol manipulation. Lesion-specific detectability was not assessed and warrants prospective follow-up.

CONCLUSIONS

Radiation dose and image quality are decoupled in neck CT. Scanner type, not dose, is the primary determinant of diagnostic quality. These findings support **scanner-specific protocol optimization** with the potential to **reduce patient dose by 30–50%** without compromising diagnostic capability, providing a replicable framework for evidence-based ALARA implementation across radiology departments.

